


WELMEC 11.6  
2017

# WELMEC

European Cooperation in Legal Metrology

## Modular evaluation of Gas meters and Volume Conversion Devices

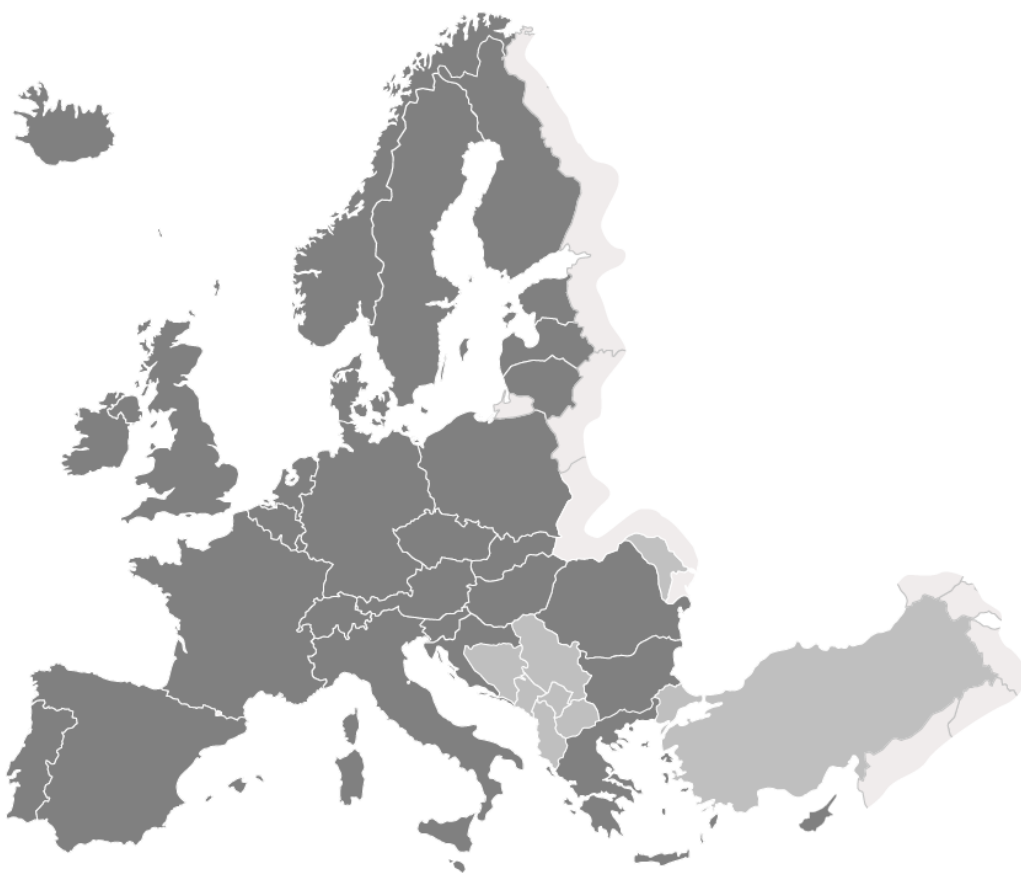

# WELMEC

European Cooperation in Legal Metrology

WELMEC is a cooperation between the legal metrology authorities of the Member States of the European Union and EFTA.

This document is one of a number of Guides published by WELMEC to provide guidance to manufacturers of measuring instruments and to Notified Bodies responsible for conformity assessment of their products.

The Guides are purely advisory and do not themselves impose any restrictions or additional technical requirements beyond those contained in relevant EU Directives.

Alternative approaches may be acceptable, but the guidance provided in this document represents the considered view of WELMEC as to the best practice to be followed.

Published by:  
WELMEC Secretariat

E-mail: [secretary@welmec.org](mailto:secretary@welmec.org)  
Website: [www.welmec.org](http://www.welmec.org)

## Contents

|     |   |    |
|-----|---|----|
| 1.  | Foreword .....  | 4  |
| 2.  | Scope .....   | 5  |
| 3.  | Definitions, abbreviations and symbols .....  | 6  |
| 4.  | Evaluation procedure of the parts .....   | 7  |
| 4.1 | Application .....   | 7  |
| 4.2 | Test requirements .....   | 7  |
| 4.3 | Evaluation .....  | 8  |
| 5.  | Certificates .....  | 9  |
| 5.1 | EC or PC .....  | 9  |
| 5.2 | TEC .....   | 9  |
| 5.3 | Revision of certificates .....  | 10 |
|     | Annex A - General requirements for gas meters and volume conversion devices .....                                   | 11 |
|     | Annex B - Technical requirements for volume conversion devices .....  | 12 |
|     | B.1 Calculator .....  | 12 |
|     | B.2 Pressure transducers .....  | 12 |
|     | B.3 Platinum resistance thermometer sensors .....   | 12 |
|     | B.4 Temperature transducers .....   | 12 |
|     | Annex C - Technical requirements for calculators and calculating/indicating devices for electronic gas meters ..... | 13 |
|     | C.1 Construction requirements .....   | 13 |
|     | C.2 Overview of requirements and applicable evaluation tests .....  | 13 |

## 1. Foreword

Gas meters and volume conversion devices are often constructed from separate parts. Those parts are produced by different Original Equipment Manufacturers (OEMs), in this document referred to as “producers”.

This document provides guidance on the evaluation of the above mentioned parts of ~~a~~ gas meters and electronic volume conversion devices.

This WELMEC guide 11.6 is used in combination with

- WELMEC guide 8.8, which provides guidance on the general and administrative aspects of the voluntary system of modular evaluation of a measuring instrument.
- WELMEC guide 7.2, which provides guidance on software requirements and validation

Other references:

- EN 12405-1/A2 (2010) “Gas meters – Conversion devices – Part 1: volume conversion”
- OIML R 137-1&2 (2012) Gas meters, Part 1: Metrological and technical requirements, Part 2: Metrological controls and performance tests

## 2. Scope

This guide covers the following:

- electronic volume conversion devices (EVCD's) type 2, as described in definition 3.1.18.2 of the EN 12405-1/A2, with the parts pressure transducers, temperature transducers and calculators;
- calculating devices or calculators including indicating devices (see 3.1.5, 3.1.6 and 6.3 of OIML R 137-1&2) of electronic gas meters, which are intended to be connected via a physical connection to the measuring part.

Parts of electronic volume conversion devices type 1 or parts of mechanical conversion devices are not under the scope of this document. Also parts of mechanical gas meters are not under the scope of this document.

Even if modular evaluation is used, the manufacturer shall apply for a conformity assessment procedure for the complete measuring instrument.

It should be noted that it is the responsibility of the manufacturer of the complete instrument to be able to demonstrate the conformity to all applicable requirements of the MID even in case the modular evaluation is used.

This guide covers only issues related to the MID. The part may bear the CE marking according to European directives other than the MID and the EC or PC number, but it cannot bear the supplementary metrology marking and Notified Body number relating to the MID.

Only a complete measuring instrument (or sub-assembly if foreseen in the MID) may bear the supplementary metrology marking and Notified Body number relating to the declaration of conformity to the MID.

### 3. Definitions, abbreviations and symbols

The definitions of the EN 12405-1/A2 and OIML R 137-1&2 apply to this guide together with the definitions given in WELMEC guide 8.8 and 7.2.

Abbreviations:

|                   |  |
|-------------------|--|
| MI                | Measuring Instrument   |
| Part              | A part of a MI which performs a specific function and can be evaluated separately.   |
| Checking facility | facility incorporated in a measuring instrument which enables significant faults to be detected and acted upon                         |
| MID               | MID, directive 2014/32/EU  |
| NB                | Notified Body  |
| TEC               | Type- or Design examination certificate  |
| EC                | Evaluation Certificate as defined in WELMEC guide 8.8  |
| PC                | Parts Certificate as defined in WELMEC guide 8.8   |
| EN 12405-1/A2     | EN 12405-1:2005+A2:2010 “Gas meters – Conversion devices – Part 1: volume conversion”  |
| OIML R 137-1&2    | “Gas meters”, Edition 2012,<br>Part 1: Metrological and technical requirements,<br>Part 2: Metrological controls and performance tests |

## 4. Evaluation procedure of the parts

For the evaluation the following procedure should be followed.

### 4.1 Application

There shall be a written application from the producer of the part for an EC or PC. The application shall contain the following: Producers name and address;

- A declaration that the part cannot be disturbed or fraudulently manipulated through its interfaces without being made evident;
- A declaration that the producer is aware of his obligations as specified in WELMEC guide 8.8, specifically related to the availability of the technical documentation;
- Complete technical documentation in accordance with article 18 of the MID, for example but not limited to:
  - General description of the type, and explanations necessary to understand the functioning of the part;
  - Technical documentation to ensure consistent production;
  - Description and characteristic data of the part;
  - Description of the checking facilities of the part;
  - Information on compatibility in respect to interfaces, power supply etc.
  - Software description, communication protocols, means for securing the software;
  - Information concerning special cases (if applicable), such as but not limited to:
    - Special operating conditions;
    - Reaction of the part to significant faults;
    - Functioning of the part after switch on.
  - A declaration of conformity stating that the hardware of the part complies with the relevant parts of the applicable directives, in particular with the EMC directive.

### 4.2 Test requirements

#### 4.2.1 Technical requirements

The part shall comply with the technical requirements as specified in relevant Annexes A, B and C.

#### 4.2.2 Requirements concerning software

The legally relevant software running on the part shall be tested in accordance with WELMEC guide 7.2: Software Guide (Measuring Instruments Directive 2014/32/EU), risk class C.

The correct functioning of the checking facilities may be tested by means of simulation.

In the case that the part is not equipped with a display, the software identification should be transmitted to another part of the measuring instrument that has a display and can indicate the software identification on request.

With respect to the reliability of volume conversion devices, chapter 6.6 of EN 12405-1/A2 applies.

### **4.2.3 Requirements concerning markings**

The part should either be inscribed with the following markings or these marking should be permanently visible on the display or a combination of both:

- EC or PC number of the device
- Producers identification mark, trademark or name
- Type designation
- Year of manufacture
- Serial number

The EC should state the position of the markings or refer to drawings that indicate the position.

## **4.3 Evaluation**

The test institute shall evaluate whether

- the documentation is confirmed to be in accordance with article 18 of the MID;
- the part is confirmed to be constructed in accordance with the documentation, in particular if the part is equipped, when applicable, with a clearly readable display, a properly operating legally relevant software, and the necessary checking facilities;
- the part is confirmed to be in accordance with the test requirements as specified in chapter 4.2.

The test institute shall issue an Evaluation Report (ER) that specifies the examinations and tests that have been performed and what the outcome of the examinations and tests were.

If the part complies with all the applicable requirements of this guide an EC or PC can be issued.



## 5. Certificates

### 5.1 EC or PC

The EC or PC should be in compliance with WELMEC guide 8.8.

In particular the EC or PC should contain:

- a description of the legally relevant characteristics of the part, including its compatibility with other devices or parts
- environmental conditions
- rated operating conditions
- a description how the software identification can be obtained
- documentation that allows the conformity of the part including the software to be checked
- a reference to the applied harmonized standard or normative document, the WELMEC 7.2 and this WELMEC 11.6 including a date reference;
- a reference to the *Evaluation Report* or *Test Report* with the appertaining test data.

### 5.2 TEC

There are two administrative ways for including a part in the TEC:

1. All references and complete description of a specific type of a part are included in the TEC of the measuring instrument, or
2. The modular approach is used
  - to allow the possibility of using parts with an EC or PC by making reference to that EC or PC
  - with the possibility of a general statement concerning the use of any part with a PC, under the condition that the requirements for the compatibility of that part with other parts are met.

Option 2 is only possible in case the EC's or PC's are issued by a test institute that can also act as a Notified Body under module B of the MID (MI-002).

#### 5.2.1 Wording in the TEC of the MI

In the application for a type-examination certificate the manufacturer of the MI may apply for the possibility of using any part evaluated under this guide.

If the manufacturer requests a general statement for the use of any part evaluated under this guide with a PC, the following conditions should be stated in the TEC:

- The part has a PC issued by a test institute that can also act as a Notified Body under module B of the MID (MI-002);
- The connection shall be made in such a way that the presentation of the results meets the essential requirements of the MID; and
- The connection shall be made through the interfaces with the specified protocols as mentioned in the TEC, and/or the PC.
- The connection to the part is secured as mentioned in the TEC, and/or the PC.

### **5.3 Revision of certificates**

The applicant shall keep the Notified Body that has issued the TEC or EC or PC informed of all modifications to the instrument or part that may affect the conformity of the instrument with the (essential) requirements or the conditions for validity of the certificate.

Where such changes influence conformity with the essential requirements or the prescribed conditions for use of the instrument or part an addition to the TEC or revision of the EC or PC is necessary.

## Annex A –General requirements for gas meters and volume conversion devices

The producer shall specify the upper temperature limit and the lower temperature limit from any of the values in table mentioned down:

|                         | Temperature limits |        |        |        |
|-------------------------|--------------------|--------|--------|--------|
| Upper temperature limit | 30 °C              | 40 °C  | 55 °C  | 70 °C  |
| Lower temperature limit | 5 °C               | -10 °C | -25 °C | -40 °C |

A minimum temperature range is 50 °C for the climatic environment.

A minimum temperature range of measured gas is 40 °C.

## **Annex B - Technical requirements for parts of volume conversion devices**

The different parts of the conversion device type 2 are examined as indicated below in chapter B.1 up to B.4.

### **B.1 Calculator**

The calculator is examined in accordance with the EN 12405-1/A2, chapter A.1.3. The maximum permissible errors are stated in the EN 12405-1/A2, Annex A.

### **B.2 Pressure transducers**

The pressure transducers are examined in accordance with the EN 12405-1/A2, Annex B.

The performance criteria are stated in the EN 12405-1/A2, chapter B.4.

### **B.3 Platinum resistance thermometer sensors**

The platinum resistance thermometer sensors are examined in accordance with the EN 12405-1/A2, Annex C.

The maximum permissible errors are stated in the EN 12405-1/A2, chapter C.4.

### **B.4 Temperature transducers**

The temperature transducers are examined in accordance with the EN 12405-1/A2, Annex D.

The maximum permissible errors are stated in the EN 12405-1/A2, chapter D.4.

## **Annex C - Technical requirements for calculators and calculating/indicating devices for electronic gas meters**

The definitions of a “calculator” and of an “indicating or displaying device” are mentioned in OIML R 137-1&2, articles 3.1.5 and 3.1.6.

### **C.1 Construction requirements**

The construction requirements of a “calculator” and of an “indicating or displaying device” are mentioned in OIML R 137-1&2, article 6.1 and 6.2. The following items shall be assessed:

- Materials
- Soundness of cases
- Protection against external interference
- Connections between electronic parts
- Components
- Zero flow

The manufacturer has to provide documentation on the constructional methods which are applied for the connection to other parts.

The EC or PC shall give information about the possibility to handle bi-directional flow (if applicable). In that case also the method shall be described.

If applicable, a dedicated power source of a “calculator” and of an “indicating or displaying device” shall have a lifetime of at least five years. After 90 % of its lifetime an appropriate warning shall be shown.

Relevant provisions of article 6.3 of OIML R 137-1&2 for electronic indicating device shall be met. In addition, the indicating device shall be able to record and display the indicated quantity of gas corresponding to at least 8000 hours of operation at the maximum flow rate  $Q_{max}$ , without returning to the original reading.

The quantity corresponding to the least significant digit shall not exceed the quantity of gas passed during one hour at  $Q_{min}$ .

Metered quantity shall be displayed in cubic metre, or in kilogram.

### **C.2 Overview of requirements and applicable evaluation tests**

The correct functioning of the calculator and/or the calculating / indicating device may be tested by means of simulation.

The following types of interfaces between the measuring part and the calculator and/or calculating/indicating device can be applied as indicated below, with the appertaining fractional error:

| Connection between measuring part and calculator and/or calculating / indicating device                               | fractional error |
|---|------------------|
| Pulses  | 0,00% *)         |
| Digital, serial communication   | 0,00% **)        |
| Rotating movement, which is translated into pulses (for the resolution of the pulses, see WELMEC 11.1, chapter 2.4.4) | 0,00% *)         |

\*) A deviation of 1 pulse may occur due to the applied test method (running start and stop).

\*\*) Apart from rounding and resolution issues.

The fractional error is the contribution of the part to the total error (MPE) of the complete measuring instrument.

Remark: the analogue input can be used for example in case of an additional temperature sensor.

The calculator and/or the calculating / indicating device is examined in accordance with paragraph 5.13.7 of the OIML R 137-1&2, while the limits are applied as indicated in Table 4 and 5.

The software shall be tested conform WELMEC Guide 7.2.

In case of digital transmission the correctness of the transmission shall be checked by the calculator or calculating/indicating device, by checking all implemented protection mechanisms.

In case of pulse transmission the correctness of this transmission shall be checked, as indicated in the OIML R 137-1/2, chapter 6.7.1. Specific pulse characteristics including the acceptable highest pulse frequency by the calculating / indicating device shall be mentioned in the EC or PC.

Remark: if a specific pulser is applied, it can be included either in the examination of the measuring part or in the examination of the calculating / indicating device.

If a correction device is included this has to be examined (see R 137-1/2 chapter 5.3.3).

If a temperature compensation is applied the temperature sensor shall be tested in combination with the calculating / indicating device.

The *Evaluation Report* or *Test Report* shall contain the test data from all the above mentioned relevant tests.